Gel Ovations
Pressure Care Products

Instruction Guide

Dimensional & Flat Gel
Pressure Relief & Positioning Products

Wheelchair and Mobility Accessories

Manufacturer:
Gel Ovations Europe Ltd
Charlton Road
Bristol BS10 6NF
United Kingdom

Contents

Intended Use 4
Dimensional, Dimensional Gel Plus, Ripple & Flat Gel Pads 5
AirGel Cushions 7
Dimensional Gel Spinal Pads 9
SlingGel 11
Gel Donuts 13
HeelGel Pressure Relief Pads 15
Arm Rest Pads & Trough Liners – G Series Arm Pads 17
Strengthening Plates For 314G & 316G Arm Pads 18
TMS & GWT Series Arm Pads 19
8TMS and 13TMS Tracking 21
GT Series Arm Pads & Accessories 23
Trough Liners 25
Gel Modular Trough Side 27
Gel Knee Protectors 29
Foot Protector Covers 31
Adjustable Foot Bucket 33
Foot Boxes & Aqua Footboxes 35
Full Length Leg Protectors 37
Gel Calf Support Panels 39
NeckGel 41
Headrests, Laterals & Elbow Pads 43
Stick-On Pads 45
GelGripz 47
Wraps and Covers 49
Permobil Compatible Gel Accessories 51
Footrest Protectors 54
Gel Hip Guides & Mounting Bracket 56
Gel Knee Adductors, Stump Pads & Elbow Stops 58
Knee Support Pads for Centre Mount Leg Rests 60
Universal Fixed Elbow Stops 62
Gel Calf Support Trough – Instructions for Use 64
Gel Lateral Hardware, Lateral Pads & Accessory Clamps 66
Gel Adjustable Forehead Stabiliser, Head Rests & Accessories 68
Shower Chair & Bathroom Accessories 71
Gel Ocean Shower Chair Soft Neoprene Back Rest 73
Gel Ovations Toilet Seat and Shower Chair Overlay 75
Horseshoe Commode Overlays & Universal Toilet Seat Pads 77
Aqua Harnesses & Aqua 2 and 4 Point Belts 79
Made to Measure Products & Customisation Service 82
Surgical Pressure Care Products 83
Warranty 84

This instruction guide does not replace clinical judgement.

Products should be selected following assessment by an appropriately trained healthcare professional.

Users at risk of pressure injury should continue to receive regular repositioning.

Intended Use

Gel Ovations pressure relief and positioning products are intended to assist with pressure redistribution, comfort, positioning and protection in seating, mobility and healthcare environments. Products should be selected following individual clinical assessment, where appropriate.

Please retain product labels and batch information for future traceability and incident reporting purposes.

Products should not be used where clinical assessment identifies that an alternative pressure management solution is required.

Products are intended for single-user use unless appropriately decontaminated in accordance with local infection control procedures.

Instructions for Use

- For Dimensional Gel and Dimensional Gel Plus products, always position the circular cell side of the gel against the user's skin or pressure area. This maximises the pressure redistribution properties of the product.
- Ensure the product is positioned correctly and lies flat before use.
- Products should be used on a stable seating or support surface.
- Whatever pressure care system is used, ensure that it is suitable for the individual user's needs and prescribed or recommended by a qualified healthcare professional where appropriate.
- Regular skin inspection is recommended, particularly for users with reduced sensation, limited mobility or high-risk pressure care needs.
- Shear and moisture can contribute to skin damage and should be minimised where possible.
- Products should be regularly inspected for signs of wear, puncture, tearing or degradation.
- Discontinue use if the product becomes damaged or compromised.
- Weight Limit: 40 Stone (254kg).

Cutting & Customisation

- Dimensional Gel, Dimensional Gel Plus, Ripple Gel and Flat Gel Pads may be cut to the required size or shape where appropriate.
- Use a good quality pair of scissors when cutting the gel.
- Following cutting, apply talc (baby powder) to the cut edges to reduce surface tackiness.
- Once customised, we highly recommend using an appropriate vapour permeable (VP) cover such as Dartex or Star Tex Fabric.
- The gel material is non-fluid and will not leak if cut or submerged in water.

Cleaning & Maintenance

- Remove any surface contamination or debris before cleaning.
- Gel surfaces may be cleaned using approved household or hospital-grade sanitising cleaners or detergents in accordance with local infection prevention and control guidelines.
- Wipe all surfaces thoroughly and ensure cleaning residue is removed where appropriate.
- Allow products to fully dry before reuse or storage.
- Do not expose products to excessive heat or sharp objects.

Cleaning of Covers

- Remove any spillage or debris from the cover surface before cleaning.
- Clean covers using a Trust-approved or hospital-approved cleaning agent in accordance with local infection control procedures.
- Rinse covers using clean water following chemical cleaning to minimise chemical residue build-up.
- Prolonged exposure to moisture or chemical residue may increase the risk of abrasion damage or strike-through.
- Always follow the cover manufacturer's cleaning instructions and recommended dilution rates for cleaning chemicals.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.
- Do not fold or place heavy objects on the gel for extended periods where possible.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, user weight, cleaning regime and environment.

AirGel Cushions

(AB16162C, AG18162C)

Intended Use

AirGel Cushions are designed to assist with pressure redistribution, comfort and postural support for wheelchair users and individuals seated for prolonged periods. Products should be selected following individual clinical assessment where appropriate.

Instructions for Use

- Position the AirGel Cushion centrally on the seating surface with the cover correctly fitted.
- Ensure that the cushion is stable and does not move during use.
- If the cushion contains adjustable air sections, ensure the cushion is inflated to the appropriate level for the user's comfort and support requirements.
- Do not overinflate the air chambers.
- Check inflation levels regularly as air pressure may alter over time.
- Ensure that the user is positioned correctly on the cushion and that posture is reassessed regularly.
- The cushion should be used with an appropriate cover where supplied.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, puncture, air loss or damage.
- Discontinue use if the cushion becomes damaged or unable to maintain inflation.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Skin should be inspected regularly, particularly for users with reduced sensation or mobility.
- Shear and moisture can contribute to skin damage.
- Do not place near sharp objects or expose to excessive heat.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Wipe clean using a household or hospital-grade sanitising cleaner in accordance with local infection control guidelines.
- Covers should be cleaned according to their individual care label instructions.
- Ensure the product is fully dry before reuse.
- Do not machine wash air components unless specifically stated.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and sharp objects.
- Avoid prolonged exposure to extreme temperatures.
- Do not store the product folded tightly or under heavy objects for extended periods.

Inspection

Before each use, check:

- Cushion inflation level
- Valves and air chambers
- Cover condition
- Signs of puncture, wear or degradation.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, user weight, cleaning regime and environment.

Dimensional Gel Spinal Pads

(3105D, 3125D, 3145D, 3165D, 3185D, 3205D)

Intended Use

Dimensional Gel Spinal Pads are designed to provide pressure redistribution, comfort and postural support to spinal or lateral support areas within seating systems and wheelchairs. Products should be selected and positioned following individual assessment where appropriate.

Instructions for Use

- Ensure that the surface where the Spinal Pad is to be fitted is clean, dry and free from dust, grease or debris before application.
- Position the Stick-on Loop hook and loop fastening strip provided in the desired location and apply firm pressure to ensure good adhesion.
- Allow the adhesive backing sufficient time to bond securely to the surface before use.
- Press the Spinal Pad firmly into its final position ensuring it is securely attached.
- Check positioning and security of attachment regularly during use.
- Ensure the pad does not interfere with the safe operation or adjustment of the seating system.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes loose, damaged or compromised.
- Ensure the adhesive hook and loop fastening strip remains securely attached before each use.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and postural support.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Wipe clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Secure attachment of hook and loop fastening fixing
- Correct positioning
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

(GSP140707, GSP140808, GSP140810, GSP141010, GSP141212, GSP380810, GSP381010, GSP381212, GSP1414)

Intended Use

SlingGel products are designed to be used within patient transfer slings to assist with pressure redistribution, comfort and skin protection during patient transfers. Products are intended to help reduce pressure on vulnerable areas and improve comfort during hoisting procedures.

Instructions for Use

- Position the SlingGel in the vulnerable area where additional pressure redistribution or skin protection is required.
- Ensure that the Grip Strips are facing the sling material and NOT the user's skin.
- Confirm that the SlingGel is securely positioned before commencing transfer.
- We recommend using a Slide Glove or Slide Sheet to assist with insertion or removal of the SlingGel where appropriate.
- Ensure that the SlingGel does not interfere with the safe operation of the sling or hoist.
- If the SlingGel is required to remain in situ following transfer, a risk assessment is strongly recommended.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, damage or degradation.
- Discontinue use if the product becomes damaged or compromised.
- SlingGel should only be used with compatible transfer slings and hoisting equipment.
- Ensure that the product remains securely positioned throughout use.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- SlingGel may be cleaned using approved household or hospital-grade sanitising cleaners or detergents in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse or storage.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Correct positioning of the SlingGel
- Grip Strip condition
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Gel Donuts

(CDRL, CDRS)

Intended Use

Gel Donuts are designed to assist with pressure redistribution, comfort and support. They may be used to reduce pressure on vulnerable areas where appropriate following clinical assessment. Products should be selected and used in accordance with the advice of a qualified healthcare professional where appropriate.

Instructions for Use

- Position the Gel Donut centrally on the seating surface before use.
- Ensure that the Gel Donut is positioned correctly in relation to the area requiring pressure relief.
- Ensure that the Donut is stable and does not move during use.
- The product should be used on a stable surface only.
- Regularly reassess comfort, posture and skin condition during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, damage or degradation.
- Discontinue use if the product becomes damaged or compromised.
- Incorrect positioning may reduce the effectiveness of pressure redistribution.
- Prolonged use without clinical supervision is not recommended for users with high-risk pressure care needs.
- Shear and moisture can contribute to skin damage.
- Regular skin inspection is recommended, particularly for users with reduced sensation or limited mobility.
- Do not expose the product to sharp objects or excessive heat.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Wipe clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure the product is fully dry before reuse.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Donut positioning
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight, sharp objects and excessive heat.
- Avoid prolonged exposure to extreme temperatures during transport or storage.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

HeelGel Pressure Relief Pads

(HG74)

Intended Use

HeelGel products are designed to assist with pressure redistribution, comfort and protection of the heel and vulnerable lower limb areas. Products are intended to help reduce pressure and friction in seating, lying and healthcare environments where clinically appropriate. Products should be selected and used following individual clinical assessment where appropriate.

Instructions for Use

- Position the HeelGel product so that the gel section is correctly aligned with the vulnerable area requiring pressure redistribution or protection.
- Ensure positioning systems are securely fitted where applicable.
- Ensure that the product is correctly fitted without restricting circulation.
- Regularly inspect skin condition and reposition the user in accordance with local pressure care guidelines.
- The product should be used on a clean, dry surface.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, damage or degradation.
- Discontinue use if the product becomes damaged or compromised.
- Regular skin inspection is recommended, particularly for users with reduced sensation, limited mobility or high-risk pressure care needs.
- Clinical supervision is recommended where appropriate.
- Ensure that straps or fastenings are not over-tightened.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to sharp objects or excessive heat.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Wipe clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Covers should be cleaned according to individual care label instructions where applicable.
- Ensure the product is fully dry before reuse.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Correct positioning
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight, sharp objects and excessive heat.
- Avoid prolonged exposure to extreme temperatures during transport or storage.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

(210G, 212G, 214G, 310G, 312G, 314G, 316G)

Intended Use

G Series Arm Pads and Trough Liners are designed to provide pressure redistribution, comfort and support for wheelchair armrests. Products are intended to help reduce pressure on vulnerable areas of the upper limbs during seated use.

Instructions for Use

- Ensure that the armrest or trough surface is clean, dry and free from debris before fitting.
- These arm pads are fitted using European M6 threaded fixings.
- Always ensure that the correct bolt length is used during installation.
- Bolts must not protrude into the gel section of the arm pad.
- Ensure all fixings are securely tightened before use.
- Check positioning and security of attachment regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Incorrect bolt length or installation may damage the product or reduce effectiveness.
- Ensure all fixings remain secure before use.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Secure attachment of all fixings
- Correct positioning
- Signs of wear, puncture or degradation
- Condition of saddle washers where fitted
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Strengthening Plates For 314G & 316G Arm Pads

(314GBO, 316GBO)

Intended Use

Strengthening Plates for 314G and 316G Arm Pads are designed to provide additional structural support and reinforcement for the 314G & 316G Arm Pads. The plates are intended to be fitted between the arm pad and plastic guard on the bottom of the arm pad.

(210TMS, 212TMS, 214TMS, 310TMS, 312TMS, 314TMS, 316TMS, 210GWT, 212GWT, 214GWT, 216GWT, 410GWT, 412GWT, 414GWT, 416GWT)

Intended Use

TMS and GWT Series Arm Pads are designed to provide pressure redistribution, comfort and upper limb support for wheelchair users and seating systems. Products are intended to assist in reducing pressure on vulnerable areas during seated use.

Instructions for Use

- Ensure that the armrest or mounting surface is clean, dry and free from debris before fitting.
- These arm pads are supplied with tracking, sliding T-Nuts and the appropriate bolts to assist fitting and adjustment.
- Ensure that the correct bolt length is used during installation.
- Bolts or fixings must not protrude into the gel section of the arm pad.
- Ensure all fixings are securely tightened before use.
- Check positioning and security of attachment regularly during use.
- Ensure the arm pad does not interfere with the safe operation or adjustment of the wheelchair or seating system.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Incorrect installation or bolt length may damage the product or reduce effectiveness.
- Ensure all fixings remain secure before use.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Secure attachment of all fixings
- Correct positioning
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

8TMS and 13TMS Tracking

Instructions for Use

- Secure the tracking to the G Series Arm Pads using the countersunk screws provided.
- Ensure that all screws are correctly aligned and securely tightened before use.
- Use the Slide Nuts and Dome Head Screws provided to secure the assembly to the wheelchair.
- Ensure that all fixings are fully tightened and that the tracking system is securely attached before use.
- Check the positioning and security of all fittings regularly during use.
- Ensure that the tracking does not interfere with the safe operation or adjustment of the wheelchair or seating system.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure that the correct supplied fixings are used during installation.
- Incorrect fitting or loose fixings may reduce product safety and effectiveness.
- Do not overtighten screws or fixings as this may damage the components.
- Ensure tracking remains securely fitted during use.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow components to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all fixings
- Correct positioning of tracking
- Integrity of screws, Slide Nuts and Dome Head Screws
- Signs of wear or damage.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

GT Series Arm Pads & Accessories

(408GT, 410GT, 412GT, 415GT, 208GT, 210GT, 212GT, 215GT)

Intended Use

GT Series Arm Pads and Accessories are designed to provide pressure redistribution, comfort and upper limb support for wheelchair users and seating systems. Accessories including trough pads, waterfall pads, elbow stops and hand pads are intended to improve positioning, support and user comfort.

Instructions for Use

- These arm pads are supplied with tracking, sliding T-Nuts and the appropriate bolts to assist fitting and adjustment.
- Ensure that the mounting surface is clean, dry and free from debris before fitting.
- Install the GT arm pad using the supplied fixings and ensure all components are securely tightened.
- Accessories including trough pads, waterfall pads, elbow stops and hand pads should be fitted using the relevant supplied fixings.
- Ensure all accessories are securely attached before use.
- Check positioning and security of all fittings regularly during use.
- Ensure the arm pads and accessories do not interfere with the safe operation or adjustment of the wheelchair or seating system.
- Refer to the latest product brochure for accessory order codes and compatible product configurations.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure that the correct supplied fixings are used during installation.
- Incorrect fitting or loose fixings may reduce product safety and effectiveness.
- Ensure all T-Nuts, bolts and accessories remain securely fitted before use.
- Do not overtighten fixings as this may damage the components.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow components to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all fixings and accessories
- Correct positioning of arm pads and accessories
- Integrity of tracking, T-Nuts and bolts
- Signs of wear, puncture or damage
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Trough Liners

(OTLM, OTLL)

Intended Use

Gel Trough Liners are designed to provide pressure redistribution, comfort and upper limb support within wheelchair trough arm systems and specialist seating environments.

Instructions for Use

- Ensure that the trough arm surface is clean, dry and free from dust, grease or debris before fitting.
- Gel Trough Liners are supplied with hook and loop fastening attached to the underside of the gel liner.
- Ensure that the corresponding hook and loop fastening is securely attached to the trough arm surface before fitting the liner.
- Position the liner correctly within the trough arm and apply firm pressure to secure it in place.
- Check positioning and attachment regularly during use.
- Ensure the liner does not interfere with the safe operation or adjustment of the wheelchair or seating system.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure the hook and loop fastening attachment remains securely fixed before use.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and support.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Secure attachment of hook and loop fastening fixing
- Correct positioning of the liner
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Gel Modular Trough Side

(2FTS10, 2FTS12, 2FTS14, 3FTS10, 3FTS12, 3FTS14, 3FTS16)

Intended Use

Gel Modular Trough Sides are designed to provide additional upper limb positioning, support and pressure redistribution when used in conjunction with compatible Gel Ovations Arm Pads and trough systems.

Instructions for Use

- All appropriate screws and Slide Nuts required for fitting are provided.
- Ensure that the arm pad or trough surface is clean, dry and free from debris before fitting.
- Fit the Gel Modular Trough Sides using the supplied screws and Slide Nuts.
- Ensure all fixings are securely tightened before use.
- Check positioning and security of attachment regularly during use.
- Ensure that the trough sides do not interfere with the safe operation or adjustment of the wheelchair or seating system.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure that the correct supplied fixings are used during installation.
- Incorrect fitting or loose fixings may reduce product safety and effectiveness.
- Ensure all Slide Nuts and screws remain securely fitted before use.
- Do not overtighten fixings as this may damage the components.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all fixings
- Correct positioning of trough sides
- Integrity of screws and Slide Nuts
- Signs of wear or damage
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

Gel Knee Protectors

Swing Away (KBM, KBMT, KBMB)

Elevating Leg Rests (KBE, KBET)

Intended Use

Gel Knee Protectors are designed to provide pressure redistribution, comfort and protection to vulnerable knee areas within wheelchair leg rest and swing away support systems.

Instructions for Use – Swing Away Models (KBM, KBMT, KBMB)

- These pads are supplied with clamps designed to fit 22mm (7/8") to 25mm (1") tubing.
- If fitting to smaller diameter tubing, a suitable sleeve may be required.
- Ensure that all clamps are securely tightened before use.
- Check positioning and security of attachment regularly during use.
- Ensure the product does not interfere with the safe operation or adjustment of the wheelchair.

Instructions for Use – Elevating Leg Rest Models (KBE, KBET)

- The Gel Knee Protector buttons for elevating leg rests are designed to fit at the upper front pivot point of most standard elevating leg rests.
- Begin by removing the existing bolt and nut from the elevating leg rest pivot joint.
- Some wheelchair manufacturers may require removal of a plastic cover before fitting.
- Replace the removed bolt with one of the supplied bolts, selecting the appropriate length.
- If the original bolt is thicker than those supplied, fit the provided steel spacers over the new bolt before reinserting into the pivot joint.
- Refit the plastic back cover over the bolt where applicable.
- Screw the Gel Knee Protector securely onto the end of the bolt.
- Replace any removed covers following installation.
- Ensure all fixings are securely tightened before use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure that all clamps, bolts and fittings remain securely tightened before use.
- Incorrect fitting may reduce product safety and effectiveness.
- Clinical supervision is recommended for users with high-risk pressure care needs.

- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all clamps, bolts and fixings
- Correct positioning of the Gel Knee Protectors
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

Foot Protector Covers

(GFPC, GPPCA, GFPCS, GFPCSQ)

Intended Use

Foot Protector Covers are designed to provide pressure redistribution, comfort and protection for wheelchair footplates and vulnerable foot areas during seated use.

Instructions for Use – GFPC / GFPCS

- Position the plastic receiver onto the footplate in the desired location.
- Mark the fixing position using a marker pen or equivalent.
- Drill the required holes into the footplate.
- Secure the receiver into position using the bolts provided.
- Ensure all fixings are securely tightened before use.
- Check positioning and security of attachment regularly during use.

Instructions for Use – GFPCA / 510GFPCA

- Fit the plastic receiver as described above.
- Ensure that both surfaces are clean, dry and free from dust or grease before fitting.
- For best results, clean the mounting surface using a spirit-based cleaning agent.
- Allow the surface to fully dry before application.
- Apply the foot pad using firm and even pressure.
- Ensure the pad is securely attached before use.

Instructions for Use – GFPCSQ

- Position the footplate overlay over the entire footplate covering both the upper and lower surfaces.
- Secure the overlay into position using the sewn-in hook and loop fastening straps.
- Ensure the overlay is securely fitted and does not move during use.
- Check positioning and attachment regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all fixings, hook and loop fastening straps and adhesive fittings remain securely attached before use.
- Incorrect fitting may reduce product safety and effectiveness.
- Clinical supervision is recommended for users with high-risk pressure care needs.

- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all fixings and straps
- Correct positioning of the product
- Signs of wear, puncture or degradation
- Integrity of adhesive surfaces where applicable
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

Adjustable Foot Bucket

(AFBHO)

Intended Use

The Adjustable Foot Bucket is designed to provide positioning, support and protection for the feet when fitted to compatible wheelchair footplates.

Instructions for Use

- Position the Adjustable Foot Bucket onto the footplate in the desired location.
- Mark the fixing position using a marker pen or equivalent.
- Drill the required holes into the footplate.
- Secure the foot bucket into position using appropriate bolts and fixings.
- Ensure all fixings are securely tightened before use.
- Adjust the angle of the foot bucket to suit the individual user requirements.
- Check positioning and security of attachment regularly during use.
- Ensure the foot bucket does not interfere with the safe operation of the wheelchair.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts and fixings remain securely tightened before use.
- Incorrect fitting may reduce product safety and effectiveness.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Do not overtighten fixings as this may damage components.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all fixings
- Correct positioning and angle adjustment
- Signs of wear or damage
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

(SSF114, SSF116, SSF118, SSF120, SSF122, SSF116RS, SSF118RS, SSF120RS, SSFCD116, SSFCD118, SSFCD120, SSF116A, SSF118A, SSF118ARS)

Intended Use

Foot Boxes and Aqua Footboxes are designed to provide positioning, support, comfort and pressure redistribution for the lower extremities during wheelchair or shower chair use. Products are intended to help support posture, improve comfort and protect vulnerable areas of the feet and lower legs.

Instructions for Use – Soft Sided Foot Boxes

- Select the correct size Foot Box for the wheelchair and user.
- Position the Foot Box securely on the wheelchair footrests.
- Use the supplied hook and loop fastening straps to secure the Foot Box around the wheelchair leg rests.
- Ensure the Foot Box is securely fitted and does not move during use.
- For Foot Boxes without a central divide, position the additional rear flap underneath the wheelchair cushion for additional stability.
- Check positioning and security regularly during use.
- For further Product Information and videos, visit www.gelovationseurope.com.

Instructions for Use – Aqua Footboxes

- Position the Aqua Foot Box securely behind the occupant's lower extremities, legs and feet to provide support and comfort.
- Adjust the Foot Box as necessary to optimise positioning and stability.
- Ensure that the Foot Box does not interfere with the safe operation of the wheelchair or shower chair.
- Check positioning regularly during use.
- Where used for postural or clinical support, use in accordance with healthcare professional guidance where appropriate.
- Water Exposure & Maintenance – Aqua Footboxes
- After each use, dry the surface of the Foot Box to prevent water accumulation.
- Do not allow water to remain within the Foot Box for prolonged periods.
- To remove excess water, tip the Foot Box on its side and allow water to drain away.
- If the Foot Box becomes saturated or waterlogged, allow it to fully dry before reuse.
- Ensure the product is fully dry before storage.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, damage or degradation.
- Discontinue use immediately if structural damage, water penetration or material failure is identified.
- Do not attempt to repair damaged products.
- Ensure the product remains securely positioned during use.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose products to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow products to fully dry before reuse or storage.
- Do not machine wash gel components unless specifically stated.

Inspection

Before use, check:

- Secure attachment of all straps and fittings
- Correct positioning of the Foot Box
- Signs of wear, puncture or degradation
- Water ingress or saturation where applicable
- Cleanliness and integrity of the product.

Storage & Transport

Store in a clean, dry environment away from direct sunlight and excessive heat.

Avoid prolonged exposure to extreme temperatures during storage or transport.

Do not store products when wet.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Full Length Leg Protectors

(FLGP10, FLGP12, FLGP14)

Intended Use

Full-length leg protectors are designed to provide pressure redistribution, comfort and protection to vulnerable lower limb areas within wheelchair and seating environments.

Instructions for Use

- These leg protectors are supplied with clamps designed to fit tubing from 22mm (7/8") to 25mm (1") diameter.
- Position the leg protector in the desired location on the wheelchair frame or leg support tubing.
- Attach the supplied clamps around the tubing and tighten securely.
- Ensure all fixings are fully tightened before use.
- If fitting to tubing smaller than 22mm (7/8") diameter, suitable sleeving may be required.
- Check positioning and security of attachment regularly during use.
- Ensure the product does not interfere with the safe operation or adjustment of the wheelchair.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all clamps and fixings remain securely tightened before use.
- Incorrect fitting may reduce product safety and effectiveness.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all clamps and fixings
- Correct positioning of the leg protectors
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

Gel Calf Support Panels

(GHS, GHSP, GHSB, GHSBX, GHS-2, GHSP-2, GHSB-2, GHSBX-2)

Intended Use

Gel Calf Support Panels are designed to provide pressure redistribution, comfort and lower limb support for wheelchair users. Products are intended to assist with calf positioning and help protect vulnerable areas during seated use.

Instructions for Use

- Attach the Gel Calf Support Panel securely to the wheelchair hanger brackets using the supplied hook and loop fastening straps.
- Ensure that all hook and loop fastening straps are securely fastened before use.
- Where fitted, use the positioning straps located at the top of the calf support panel to achieve the most appropriate position for the individual user.
- Adjust positioning to optimise support, comfort and lower limb alignment.
- Check positioning and attachment regularly during use.
- Ensure the product does not interfere with the safe operation or adjustment of the wheelchair.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all hook and loop fastening straps and positioning straps remain securely attached before use.
- Incorrect positioning may reduce the effectiveness of support and pressure redistribution.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all hook and loop fastening and positioning straps
- Correct positioning of the calf support panel
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

NeckGel

Intended Use

The NeckGel is designed to support positioning of the head and neck to enhance comfort, assist posture and aid pressure redistribution during seated or reclined use.

Intended Users & Environment

The product is intended for use by adults and children under the supervision of an appropriate caregiver or healthcare professional in domestic, community, care home or clinical environments.

Instructions for Use

- Gently flex the NeckGel and position it under the front, side or back of the neck as appropriate for the user's needs.
- Reposition and adjust as required to achieve the desired level of support and comfort.
- Ensure that the user's airway and head position remain safe and unobstructed during use.
- Assessment by a healthcare professional is recommended for users with complex postural, positioning or pressure care needs.
- Regularly reassess positioning, comfort and skin condition during use.

Warnings & Precautions

- Do not use the product if damaged, punctured or defective.
- Do not attempt repairs or modifications.
- Repeated excessive flexing or incorrect handling may damage the product.
- Ensure the product is correctly positioned before use.
- Users requiring postural support should be supervised in accordance with their individual care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- The product is not a toy.
- Do not expose the product to excessive heat, sharp objects or open flames.

Cleaning & Maintenance

- Outer covers are removable for cleaning.
- Wash covers at 30°C unless otherwise stated on the care label.
- Line dry where possible or tumble dry on a low temperature.
- Do not use bleach, harsh chemicals or abrasive cleaning agents.
- Clean gel surfaces using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all components are fully dry before reuse or storage.
- Outer Fibre Content: 95% Bamboo, 5% Lycra, 4-way stretch fabric.

Inspection

Before use, check:

- Cover condition
- Signs of wear, puncture or gel leakage
- Damaged seams or stitching
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a cool, clean and dry environment away from direct sunlight, excessive heat and sharp objects.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Traceability

Please retain the product label containing the batch number for future reference.

Product Information

Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Headrests, Laterals & Elbow Pads

(55DGHP, 77DGHP, 35DGLP, 46DGLP, 57DGLP, 67DGLP, 89DGLP, 35DGES1, 46DGES1, 57DGES1, 67DGES1, 89DGES1, AEP, DAEPC1, DAEPC)

Intended Use

Headrests, Laterals & Elbow Pads are designed to provide pressure redistribution, postural support and comfort for the head, neck, elbow and trunk within wheelchair and specialist seating systems.

Instructions for Use

- Fit the Headrest, Lateral or Elbow Pad using the supplied bolts and appropriate mounting hardware.
- Ensure that all fixings are securely tightened before use.
- Adjust positioning to provide appropriate support, alignment and comfort for the individual user.
- Ensure the product does not interfere with the safe operation or adjustment of the wheelchair or seating system.
- Check positioning and security of attachment regularly during use.
- Products are supplied with removable covers for cleaning and maintenance.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts and mounting hardware remain securely tightened before use.
- Incorrect positioning may reduce the effectiveness of postural support and pressure redistribution.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Removable covers should be cleaned in accordance with the care label instructions.
- Gel and foam components should be cleaned using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow all components to fully dry before reuse or refitting covers.

Inspection

Before use, check:

- Secure attachment of all bolts and fixings
- Correct positioning of the Headrest or Laterals
- Signs of wear, puncture or degradation
- Condition of removable covers
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

Stick-On Pads

(ESP, SESP, 34SP, 48SP, 412SP, 1575SP, 2075SP, 2012SP, 2575SP)

Intended Use

Stick-On Pads are designed to provide pressure redistribution, protection and comfort when applied to compatible wheelchair, seating or support surfaces.

Instructions for Use

- Before fitting, ensure that both surfaces are clean, dry and free from dust, grease or debris.
- For best results, clean the mounting surface using a suitable spirit-based cleaning agent.
- Allow the surface to fully dry before application.
- Position the pad carefully in the desired location.
- Apply firm and even pressure across the pad surface to ensure secure adhesion.
- Once fitted, it is not recommended to remove and re-use the pad.
- Check positioning and adhesion regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure the adhesive surface remains securely attached before use.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and protection.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure adhesion of the pad
- Correct positioning
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.
- Keep adhesive surfaces protected prior to fitting.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

(WHC4, WHC5, RHC, MFCZ, MCH4, MCH5, MCRH)

Intended Use

GelGripz products are designed to provide additional comfort, cushioning and grip enhancement for walking aids, mobility equipment handles and other contact surfaces. Products are intended to assist in reducing pressure and improving user comfort during use.

Instructions for Use

- Ensure that the walking aid handle, frame or contact surface is clean, dry and free from dust, grease or debris before fitting.
- Position the GelGripz centrally onto the handle or designated contact surface.
- Where supplied with fastening straps, zips, hook and loop fastening or adhesive backing, ensure these are fully secured before use.
- Position any seams away from the area requiring protection or pressure relief.
- Apply even pressure during fitting to ensure secure positioning.
- Ensure the product does not interfere with the safe operation, grip or braking function of the walking aid or mobility equipment.
- Check positioning and attachment regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes loose, damaged or compromised.
- Ensure GelGripz are securely fitted before use to reduce the risk of slipping.
- Do not use the product if it affects the safe handling, control or braking function of the walking aid.
- Clinical supervision is recommended where users have impaired grip strength, dexterity or balance issues.
- Regular skin inspection is recommended for users with reduced sensation or vulnerable skin.
- Keep away from sharp objects, excessive heat and open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse or storage.
- Removable covers or fabric components should be cleaned in accordance with the care label instructions where applicable.

Inspection

Before use, check:

- Secure fitting and positioning
- Condition of straps, zips, hook and loop fastening or adhesive backing
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

(THC, BCC16, BCC18, BCC20, PTW6, PTW8, SBCV, SBCPV, SBCBV, GSC5, GSC8, LHC, LPW, LLPW, TAC, KPR, KPRT, KPRQ, HLC3, GLS26, GLS32, GLS36, INVSCFP, INVSCFP1P, INVSCLP, INVSCHR, INVSCBR, INVSCBBW, GMSS, 310V, 312V, 314V, SFC1034, SFC1056, SFC107, 510VFP, 610VFP, GPSB14, GPSB16, GPSB18, GPSB20)

Intended Use

Wraps and Covers are designed to provide pressure redistribution, comfort, protection and cushioning for vulnerable body areas, wheelchair components, seating systems and mobility equipment. Products may assist in reducing pressure, friction and shear where clinically appropriate.

Instructions for Use

- Ensure the surface or body area where the product is to be fitted is clean and dry before use.
- Position the Wrap or Cover over the required area ensuring correct alignment and coverage.
- Where supplied with Velcro, straps, zips or fastening systems, ensure these are securely fastened before use.
- Position seams and fastening areas away from vulnerable skin areas wherever possible.
- Ensure the product does not interfere with the safe operation of wheelchairs, mobility aids or seating systems.
- Reposition and adjust as required to optimise comfort and protection.
- Check positioning and security regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged, loose or compromised.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and protection.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation, fragile skin or limited mobility.
- Shear and moisture can contribute to skin damage.
- Ensure straps and fastenings are secure but do not restrict circulation.
- Keep away from sharp objects, excessive heat and open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Fabric covers or removable components should be cleaned in accordance with the care label instructions.
- Ensure all cleaning residue is removed where appropriate.
- Allow products to fully dry before reuse or storage.

Inspection

Before use, check:

- Secure fitting and positioning
- Condition of straps, zips, hook and loop fastening or fastenings
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.
- Do not store products when wet.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel unless otherwise stated. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime, fitting conditions and environment.

(DP2SC10, DP3SC10, DP2SC12, DP3SC13, DP2SC14, DP2SC16, DP3SC16)

These instructions are intended to assist with the safe fitting and use of Permobil Compatible Gel Arm Pad Slip-Covers.

Intended Use

Permobil Compatible Gel Arm Pad Slip-Covers are designed to provide additional pressure redistribution, comfort and protection for compatible Permobil wheelchair arm pads.

Fitting Instructions

Step 1: Remove the arm pad assembly from the chair using a suitable screwdriver.

Step 2: Use flat screwdriver. Follow Diagram 1 instructions and gently push the tabs to separate the pad from the assembly. Push tabs in the direction of the arrows.

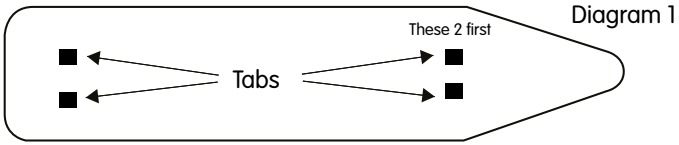

Step 3: Apply the supplied adhesive tape to the locations shown in the fitting guide on the plastic plate containing the retaining tabs. The adhesive strips should be positioned on the side facing the floor when reinstalled on the chair.

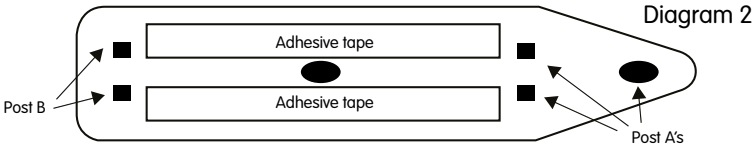

Step 4: The slip-cover contains integrated gel shaped to match the arm pad profile. Slide the pointed end of the Permobil arm pad into the slit within the slip-cover so both pointed ends align in the same direction.

Step 5: Align the three pre-punched holes in the slip-cover with Post A locations on the Permobil arm pad and carefully stretch the fabric over each post.

Step 6: Stretch the fabric evenly over the squared end of the Permobil arm pad.

Step 7: Align the two remaining pre-punched holes with Post B locations and carefully stretch the fabric over each post.

Step 8: Remove the protective backing paper from one adhesive strip while holding the fabric clear of the adhesive.

Step 9: Gently stretch the fabric to align the seam centrally with the Permobil base plate and press the fabric firmly onto the adhesive strip. If required, the fabric may be repositioned by lifting and reapplying.

Step 10: Remove the backing from the second adhesive strip and secure the remaining fabric to the exposed adhesive. Ensure taped edges do not overlap.

Step 11: Align the slip-covered arm pad over the assembly and press firmly until the retaining tabs engage securely.

Step 12: Reattach the arm pad assembly to the wheelchair using the appropriate screwdriver and fixings.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fitting or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all retaining tabs and fixings are securely engaged before use.
- Incorrect fitting may reduce the effectiveness of pressure redistribution and support.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat, sharp objects or open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Covers should be cleaned in accordance with the care label instructions.
- Clean gel surfaces using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow all components to fully dry before reuse or refitting.

Inspection

Before use, check:

- Secure fitting of the slip-cover
- Correct engagement of retaining tabs
- Signs of wear, puncture or degradation
- Adhesive attachment integrity
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

Footrest Protectors

(5PFPCS, 7PFPCS)

Intended Use

Footrest Protectors are designed to provide pressure redistribution, protection and cushioning for wheelchair footplates and vulnerable foot areas.

Instructions for Use

- Ensure that the wheelchair footplates are clean, dry and free from dust, grease or debris before fitting.
- For best results, clean the mounting surface using a suitable spirit-based cleaning agent.
- Allow the surface to fully dry before application.
- Carefully position the Footrest Protector in the desired location.
- Apply firm and even pressure across the surface to ensure secure adhesion.
- Once fitted, it is not recommended to remove and re-use the product.
- Check positioning and adhesion regularly during use.
- Ensure the product does not interfere with the safe operation of the wheelchair.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure the adhesive surface remains securely attached before use.
- Incorrect positioning may reduce the effectiveness of protection and pressure redistribution.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Keep away from sharp objects, excessive heat and open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure adhesion of the Footrest Protector
- Correct positioning
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.
- Keep adhesive surfaces protected prior to fitting.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions and environment.

Gel Hip Guides & Mounting Bracket

(HG310, HG312, HG314, HG316, HGMB)

Intended Use

Gel Hip Guides and Mounting Brackets are designed to provide adjustable lateral positioning, postural support and pressure redistribution within wheelchair and specialist seating systems.

Instructions for Use

- Gel Ovations Hip Guides are designed with 6-axis adjustability to allow flexible positioning for individual user requirements.
- Loosen the adjustment screws sufficiently to reposition the Hip Guide.
- Adjust the Hip Guide and aluminium fitting to the desired position.
- The aluminium fitting is infinitely adjustable and does not have fixed positioning points.
- Once the required position has been achieved, securely tighten all bolts and fixings.
- Ensure the Hip Guide is securely fixed before use.
- Check positioning and security of attachment regularly during use.
- Ensure the Hip Guide does not interfere with the safe operation or adjustment of the wheelchair or seating system.
- Mounting Information
- The standard Hip Guide stem is designed to fit directly into the Quickie Salsa skirt guard receiver bracket.
- For use with other wheelchair or seating systems, the Hip Guide Mounting Bracket (HGMB) may be required.
- The HGMB Mounting Bracket is supplied with T-Nuts and various bolt lengths compatible with most major wheelchair seat track systems.
- Ensure that the appropriate fixings are selected and securely tightened during installation.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all adjustment screws, bolts and fixings remain securely tightened before use.
- Incorrect positioning or installation may reduce the effectiveness of postural support and pressure redistribution.
- Clinical supervision is recommended for users with complex postural or high-risk pressure care needs.

- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all fixings and adjustment points
- Correct positioning of the Hip Guide
- Integrity of T-Nuts, bolts and mounting hardware
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

(SRABC, SRABCSC, SRASC, SRABD, SRASD, SRABF, SRASF, SRABO, SRASO, SRABE, SRASE, SRABG, SRASG, 67SRSSC, 67SRSSD, 89SRSSC, 89SRSSD, 67SRSSF, 89SRSSF, SRESD, SRESC, SRPESD, SRPESC, 67SRSSO, 89SRSSOR, 67SRSSE, 89SRSSE, 67SRSSG, 89SRSSG, 67DSSP, 89DSSP)

Intended Use

Gel Knee Adductors, Stump Pads and Elbow Stops are designed to provide postural positioning, pressure redistribution, support and protection within wheelchair and specialist seating systems.

Instructions for Use

- If using tube clamp versions, ensure that the correct size tube clamps have been selected for the wheelchair tubing.
- Many clamp sizes are available: 22mm (7/8") and 25mm (1"), Oval 33 x 27mm (1.3 x 1.07"), 28mm (1.1") and 30 – 32mm (1.18 – 1.26")
- Loosely attach the tube clamp to the wheelchair tubing.
- Slacken each clamp screw individually and adjust the Gel Adductor Pad, Stump Pad or Elbow Stop to the desired position.
- Repeat the adjustment process as required until the correct position is achieved.
- Once correctly positioned, securely tighten the tube clamp bolts and all set screws.
- Ensure all fixings are secure to prevent rotation or movement during use.
- For Flat Mount Fixing versions, use the supplied T-Nuts and screws to attach the fixing bracket to the wheelchair side rails.
- For Quick Release versions, use the lever mechanism to tighten or release the support when adjustment or removal is required.
- Fixed Position Elbow Stops (EBLSD, EBLSC) are designed to clamp directly onto wheelchair back posts.
- Ensure the correct size tube clamp is used and secure using the supplied lock screws and set screws.
- Check positioning and security of attachment regularly during use.
- Spare stump pads available 67DSSP (6 x 7"), 89DSSP (8 x 9")

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all clamp bolts, set screws and fixings remain securely tightened before use.
- Incorrect fitting or positioning may reduce the effectiveness of postural support and pressure redistribution.

- Clinical supervision is recommended for users with complex postural or high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all clamps, bolts and set screws
- Correct positioning of the support hardware
- Integrity of T-Nuts, brackets and fixing hardware
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

Knee Support Pads for Centre Mount Leg Rests

(SRCMS, SRCMS35, SRCMS46, SRCMS57, SRCMS67, SRCMS89)

Intended Use

Knee Support Pads for Centre Mount Leg Rests are designed to provide positioning support, pressure redistribution and comfort for users requiring lower limb support within wheelchair and power chair seating systems.

Instructions for Use

- These products are designed for use in conjunction with compatible wheelchair or power chair seat rail systems.
- Remove the seat rail end stop to allow access to the tracking system.
- Insert the appropriate size track nuts supplied into the seat rail tracking.
- Use the supplied Cap Head Screws to attach the Swivel Mount Receiver Bracket to the track nuts.
- Slide the Receiver Bracket along the seat rail to the desired position.
- Attach the Knee Support Pad hardware to the Swivel Mount Receiver Bracket using the Swing Away Clamp.
- Adjust the hardware positioning using suitable Allen Keys until the desired support position is achieved.
- Once correctly positioned, securely tighten all bolts, screws and adjustment points.
- Replace the seat rail end stop after fitting is complete.
- Check positioning and security of attachment regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts, track nuts, clamps and adjustment points remain securely tightened before use.
- Incorrect positioning or installation may reduce the effectiveness of postural support and pressure redistribution.
- Clinical supervision is recommended for users with complex postural or high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all track nuts, brackets and fixings
- Correct positioning of the Knee Support Pad
- Integrity of clamps and adjustment hardware
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

Universal Fixed Elbow Stops

(UESF, UESC, 35UES, 46UES, 57UES, HDESUS, HDESUL, EBLSD, EBLSC)

Intended Use

Universal Fixed Elbow Stops are designed to provide upper limb positioning, support and protection within wheelchair and specialist seating systems.

Instructions for Use – Arm Pad Mounted Versions

- These elbow pads are compatible with Gel Ovations Arm Pads that are greater than 3" (76mm) wide.
- Position the Elbow Stop in the desired location on the existing arm pad.
- Secure the Elbow Stop using the appropriate bolts and fixings.
- Ensure all fixings are securely tightened before use.
- Check positioning and security of attachment regularly during use.
- Ensure the Elbow Stop does not interfere with the safe operation or adjustment of the wheelchair or seating system.

Instructions for Use – Clamp Mounted Versions (EBLSD, EBLSC)

- These fixed-position elbow stop brackets are supplied with either a 1" (25mm) or 7/8" (22mm) clamp.
- Ensure that the correct clamp size has been selected for the wheelchair tubing.
- Position the clamp onto the wheelchair back post in the desired location.
- Adjust the Elbow Stop position as required.
- Securely tighten all clamp bolts and set screws.
- Check positioning and security of attachment regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts, clamps and fixings remain securely tightened before use.
- Incorrect positioning or installation may reduce the effectiveness of support and pressure redistribution.
- Clinical supervision is recommended for users with complex postural or high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all bolts, clamps and fixings
- Correct positioning of the Elbow Stop
- Integrity of mounting hardware
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

Gel Calf Support Trough – Instructions for Use

(DGCT, DGCP)

Intended Use

Gel Calf Support Troughs are designed to provide pressure redistribution, comfort and lower limb support when fitted to compatible wheelchair leg support systems.

Instructions for Use

- The Gel Calf Support Trough is designed to be fitted to existing wheelchair leg supports.
- Position the trough support in the desired location to provide appropriate calf support and positioning.
- Use the supplied bolts and fixings to secure the trough support into position.
- Ensure all bolts and fixings are securely tightened before use.
- Adjust positioning as required to optimise comfort, support and pressure redistribution.
- Check positioning and security of attachment regularly during use.
- Ensure the product does not interfere with the safe operation or adjustment of the wheelchair.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts and fixings remain securely tightened before use.
- Incorrect positioning or installation may reduce the effectiveness of support and pressure redistribution.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all bolts and fixings
- Correct positioning of the trough support
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

(SRRLHL, SRRLHR, 35DGLP1, 46DGLP1, 57DGLP1, 67DGLP1, 89DGLP1, SAB2D1, SAB2C1, SAB3D1, SAB3C1, SRLL2, SRLL3)

Intended Use

Gel Lateral Hardware, Lateral Pads and Accessory Clamps are designed to provide adjustable lateral positioning, postural support and pressure redistribution within wheelchair and specialist seating systems.

Instructions for Use – Lateral Hardware & Pads

- Select the appropriate left or right lateral support hardware and the required lateral pad size.
- Secure the lateral pad to the lateral hardware using the supplied bolts and fixings.
- Attach the lateral hardware to the wheelchair or mobility aid using the appropriate Accessory Clamp.
- Loosen the positioning screws on the lateral hardware to adjust the support to the desired position.
- Once the correct position has been achieved, securely tighten all screws and fixings.
- The lateral support may be swung in and out of position using the integrated lift mechanism within the hardware.
- Check positioning and security of attachment regularly during use.
- Ensure the lateral support does not interfere with the safe operation or adjustment of the wheelchair or seating system.

Instructions for Use – Lateral Link Extensions (SRLL2, SRLL3)

- Remove the existing fixing screws from the lateral hardware.
- Insert the lateral extension links to achieve the desired extension length.
- Refit and securely tighten the fixing screws.
- Check that all extension links and fixings are secure before use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts, clamps, screws and extension links remain securely tightened before use.
- Incorrect positioning or installation may reduce the effectiveness of postural support and pressure redistribution.
- Clinical supervision is recommended for users with complex postural or high-risk pressure care needs.

- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Do not expose the product to excessive heat or sharp objects.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all clamps, bolts and fixings
- Correct positioning of lateral supports
- Integrity of lift mechanisms and extension links
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

(SRAFS510, SRAFS512, SRAFS514, SRAFSRAZ, SRAFS, SCHA, SRFSMB, SRFSMBS, SRFSMBW, SRFSMBP, SRFSMBR, SRFSMBE, SRFSMBC4, SRHR15, SRHR34, SRHR5)

Intended Use

- Gel Adjustable Forehead Stabilisers, Head Rests and Accessories are designed to provide adjustable head positioning, postural support and comfort within wheelchair, shower chair and specialist seating systems.
- Compatible Headrests & Systems
- The Forehead Stabiliser may be used with Gel Ovations Headrests SRH510, SRH512 and SRH514.
- When fitting to an Ocean Shower Chair, bracket SCHA must be used.
- Square post Mounting Stems SRHR15 (15mm), SRHR34 (19mm) and SRHR5 (13mm) can be used to mount SRAFS510, SRAFS512 and SRAFS514.
- The Forehead Stabiliser may also be fitted to compatible third-party headrests using the appropriate adaptor brackets.

Instructions for Use – Forehead Stabiliser

- Set the arm length and connect the arms using the supplied socket head screw.
- Adjust the position of the Forehead Stabiliser by setting the forehead pad angle.
- Tighten the flat-head screw once the desired angle has been achieved.
- Adjust the arm angle to achieve the required support position.
- Tighten all adjustment screws securely once positioning is complete.
- Install the Gel Wraps around the arms of the Forehead Stabiliser.
- Use the 'Push to Release' button to move the Forehead Stabiliser between forward and rearward positions as required.
- Check positioning and security of attachment regularly during use.

Adaptor Brackets for Third-Party Headrests – Ball Fixing Versions

- Remove the existing headrest from the 1" (25mm) or ¾" (19mm) ball fixing.
- Position the appropriate Gel Ovations Ball Adaptor Bracket between the ball fixing and the headrest pad.
- Using the supplied screws, securely attach the adaptor bracket.
- Fit the Gel Ovations Forehead Stabiliser (SRAFS) to the adaptor bracket using the supplied screws.
- Retain all removed screws in case the original configuration is required in the future.

Adaptor Bracket – Whitmyer Style Headrests (SRFSMBW)

- Remove the two screws securing the removable lower clamp.
- Position the Whitmyer adaptor onto the welded clamp section with the longer, thinner section facing away from the headrest pad.
- Ensure the drilled and tapped fixing holes face upward.
- Use the supplied longer screws to refit and secure the clamp assembly.
- Tighten the headrest clamp securely around the welded half clamp.
- Attach the Forehead Stabiliser to the adaptor using the supplied screws.
- Retain all removed screws for future use if required.

Adaptor Brackets – R82, Permobil, Etac & Comfort Company Headrests

- Attach the correct adaptor bracket to the rear of the existing headrest using the supplied screws.
- Ensure the pre-drilled and tapped fixing holes are positioned towards the top of the headrest.
- Attach the Forehead Stabiliser (SRAFS) to the adaptor bracket using the supplied screws.
- Refer to the Product Selector or www.gelovationseurope.com for additional diagrams and fitting guidance.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all bolts, screws, clamps and adjustment mechanisms remain securely tightened before use.
- Incorrect positioning or installation may reduce the effectiveness of postural support.
- Clinical supervision is recommended for users with complex postural or high-risk support needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Ensure the Forehead Stabiliser does not obstruct breathing, visibility or emergency access.
- Do not expose the product to excessive heat, sharp objects or open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean gel and hardware components using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Fabric wraps or removable covers should be cleaned in accordance with the care label instructions.
- Ensure all cleaning residue is removed where appropriate.
- Allow all components to fully dry before reuse.

Inspection

Before use, check:

- Secure attachment of all brackets, clamps and fixings
- Correct positioning and adjustment
- Integrity of release mechanisms and moving parts
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations.

Product Information

All gel used is latex-free solid gel. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

(LPW, KPR, TAC, OTACA, INVSCFP, INVSCFP1P, INVSCLP, INVSCHR, INVSCBBW, RAZSCFP, RAZSCFPSV, RAZSCHR, RAZSCBRO, RAZSCLP, SFTSCFP, SFTSBW, SFTABW, SFTSC, ECSOC, ECBRC, ECFRP, OSPSCFP1, OSPSCFP)

Intended Use

Shower Chair and Bathroom Accessories are designed to provide pressure redistribution, comfort and protection for vulnerable areas when used with shower chairs, bathroom seating and related mobility equipment.

Instructions for Use

- Position the product around the required support surface, frame, rail or contact area.
- Secure the product using the integrated zip or hook and loop fastening fastening system.
- Ensure the product is securely fitted and positioned correctly before use.
- Position seams and fastening areas away from vulnerable skin areas wherever possible.
- Adjust positioning as required to optimise comfort and protection.
- Check positioning and attachment regularly during use.
- Ensure the product does not interfere with the safe operation of the shower chair or bathroom equipment.
- Drying & Moisture Management
- After cleaning and exposure to water, allow air to circulate fully around the product until completely dry.
- Do not store products when damp or wet.
- Ensure the product is fully dry before reuse.
- Avoid prolonged exposure to standing water or excessive moisture.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged or compromised.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and protection.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation, fragile skin or limited mobility.
- Shear and moisture can contribute to skin damage.

- Ensure zips, hook and loop fastening straps and fastenings are secure before use.
- Keep away from sharp objects, excessive heat and open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Fabric covers or removable components should be cleaned in accordance with the care label instructions where applicable.
- Ensure all cleaning residue is removed where appropriate.
- Allow products to fully dry before reuse or storage.

Inspection

Before use, check:

- Secure fitting and positioning
- Condition of zips, hook and loop fastening straps and fastenings
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.
- Do not store products when wet.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel unless otherwise stated. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime, fitting conditions and environment.

Gel Ocean Shower Chair Soft Neoprene Back Rest

(INVSCBR)

Intended Use

The Gel Ocean Shower Chair Soft Neoprene Back Rest is designed to provide additional comfort, pressure redistribution and support for users of compatible Ocean Shower Chairs and similar bathroom seating systems.

Instructions for Use

- Fully remove the existing backrest from the shower chair before fitting the product.
- Position the Gel Ocean Shower Chair Soft Neoprene Back Rest in the desired location on the chair frame.
- Secure the backrest using the supplied hook and loop fastening straps and buckle fastenings.
- Adjust the hook and loop fastening straps to achieve the required level of comfort, positioning and support.
- Ensure all buckles, clips and fastening straps are securely attached before use.
- Check positioning and attachment regularly during use.
- Ensure the backrest does not interfere with the safe operation or adjustment of the shower chair.
- Drying & Moisture Management
- After cleaning or exposure to water, allow air to circulate fully around the product until completely dry.
- Do not store the product when damp or wet.
- Ensure the product is fully dry before reuse.
- Avoid prolonged exposure to standing water or excessive moisture.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fastenings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all straps, buckles and clips remain securely fastened before use.
- Incorrect positioning may reduce the effectiveness of support and pressure redistribution.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation or limited mobility.
- Shear and moisture can contribute to skin damage.
- Keep away from sharp objects, excessive heat and open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse or storage.
- Do not use abrasive cleaning agents or harsh chemicals.

Inspection

Before use, check:

- Secure attachment of all hook and loop fastening straps, buckles and clips
- Correct positioning of the backrest
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.
- Do not store products when wet.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime, fitting conditions and environment.

Gel Ovations Toilet Seat and Shower Chair Overlay

(GTSO, GTSOM)

Intended Use

Gel Ovations Toilet Seat and Shower Chair Overlays are designed to provide pressure redistribution, comfort and skin protection when used on toilet seats, commodes and shower chairs.

Instructions for Use

- Position the overlay securely onto the toilet seat, commode or shower chair seat.
- Ensure that the non-slip material is positioned against the seating surface.
- Ensure that the vapour permeable cover surface is positioned in contact with the user.
- Secure the overlay in position using the supplied hook and loop fastening straps.
- Check that the product is stable and securely fitted before use.
- If the hook and loop fastening straps are not required, they may be carefully cut off and disposed of appropriately.
- Ensure the overlay does not interfere with the safe operation or stability of the seating equipment.
- Check positioning and security regularly during use.

Cleaning & Maintenance

- Remove any spillage, debris or contamination from the surface before cleaning.
- The vapour permeable cover may be wiped clean using soap and warm water.
- Approved household or hospital-grade sanitising cleaners may also be used in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow the product to fully dry before reuse or storage.
- Do not use abrasive cleaning agents, solvents or harsh chemicals.
- Drying & Moisture Management
- After cleaning or exposure to moisture, allow air to circulate fully around the product until completely dry.
- Do not store products when damp or wet.
- Avoid prolonged exposure to standing water or excessive moisture.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged or compromised.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and protection.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation, fragile skin or limited mobility.
- Shear and moisture can contribute to skin damage.
- Ensure the overlay remains securely positioned during use.
- Keep away from sharp objects, excessive heat and open flames.

Inspection

Before use, check:

- Secure fitting and positioning
- Condition of hook and loop fastening straps and non-slip surfaces
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel unless otherwise stated. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Horseshoe Commode Overlays & Universal Toilet Seat Pads

(DGCPCO1818, DGCPCO1820, DGTPC, DGCPC1616)

Intended Use

Horseshoe Commode Overlays and Universal Toilet Seat Pads are designed to provide pressure redistribution, comfort and skin protection when used on commodes, shower chairs and toilet seating systems.

Instructions for Use – Horseshoe Commode Overlays & Universal Toilet Seat Pads

- Position the overlay securely on top of the existing commode, shower chair or toilet seat.
- Secure the product in position using the supplied hook and loop fastening straps.
- Commode overlays include additional rear straps designed to secure around the back posts of the backrest.
- Ensure all straps are securely fastened before use.
- Check that the product is stable and correctly positioned prior to use.
- The Dimensional Gel inserts may be removed to allow the covers to be cleaned separately.
- Ensure all inserts are correctly refitted before reuse.

Instructions for Use – Universal Dimensional Gel Commode Overlay Closed Style (DGCPC1616)

- Ensure that both the existing seat surface and overlay are clean, dry and free from dust, grease or debris.
- Apply the supplied Grip Strips using firm and even pressure.
- Two Grip Strips should be applied to the existing seat surface and two to the rear of the overlay.
- Maximum adhesive strength is achieved after approximately 72 hours, with approximately 90% adhesion achieved after 24 hours.
- Check positioning and stability regularly during use.

Cleaning & Maintenance

- Remove any spillage, debris or contamination before cleaning.
- Covers may be machine washed at up to 60°C on a gentle cycle using neutral detergents.
- Adequate drying is essential for product care and maintenance.
- Air drying is the preferred drying method.
- Do not iron or press the fabric.

- Gel surfaces may be cleaned using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all components are fully dry before reuse or storage.
- Drying & Moisture Management
- After cleaning or exposure to moisture, allow air to circulate fully around the product until completely dry.
- Do not store products when damp or wet.
- Avoid prolonged exposure to standing water or excessive moisture.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, movement or damage.
- Discontinue use if the product becomes damaged or compromised.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and protection.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Regular skin inspection is recommended for users with reduced sensation, fragile skin or limited mobility.
- Shear and moisture can contribute to skin damage.
- Ensure all straps, Grip Strips and fastenings remain secure before use.
- Keep away from sharp objects, excessive heat and open flames.

Inspection

Before use, check:

- Secure fitting and positioning
- Condition of hook and loop fastening straps, Grip Strips and fastenings
- Signs of wear, puncture or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

All gel used is latex-free solid gel unless otherwise stated. Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, cleaning regime and environment.

Aqua Harnesses & Aqua 2 and 4 Point Belts

(AHS, AHM, AHL, AHXL, A2PBS, A2PBM, A2PBL, A4PBS, A4PBM, A4PBL)

Intended Use

Aqua Harnesses and Aqua 2 and 4 Point Belts are designed to provide postural positioning and support for users of compatible shower chairs and bathroom seating systems.

Important Clinical Guidance

- It is strongly recommended that the fitting, adjustment and positioning of all belts and harnesses is carried out by an appropriately trained healthcare professional.
- Products are intended for positioning support only and are not transport restraints.
- Regular user monitoring and skin inspection is recommended.

Instructions for Use – Aqua Harnesses

- Identify two suitable mounting locations for the P-clamps on the rear tubular bars of the chair facing backwards.
- These mounting points will secure the shoulder straps into position.
- Secure the fixed lock buckles to the P-clamps using the supplied nuts and bolts.
- Ensure all fixings are securely tightened before use.
- Orientate the harness correctly with the longer padded sections positioned upwards to pass comfortably over the user's shoulders.
- Feed the shoulder straps through the respective buckles but do not fully tighten at this stage.
- Attach the lower harness straps to the lower rear tubular bars of the seat using the supplied slide buckles.
- Adjust the straps to achieve the required level of support and positioning.
- Ensure the padded sections remain in contact with the user during use.
- Once the correct position is achieved, securely fasten and tighten all straps and buckles.
- Check positioning and attachment regularly during use.

Instructions for Use – Aqua 2 & 4 Point Belts

- Wrap the belt fitting straps around the lower rear tubular bars of the seat and/or backrest.
- Feed the straps through the supplied slide buckles and adjust accordingly.
- For 4-Point Belts, repeat the process using the additional straps positioned along the sides of the seat as required.
- Ensure all straps and buckles are securely fastened before use.
- Adjust positioning to optimise comfort, support and postural alignment.
- Check positioning and attachment regularly during use.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, loose fixings or damage.
- Discontinue use if the product becomes damaged or compromised.
- Ensure all straps, buckles, clamps and fixings remain securely attached before use.
- Incorrect fitting or positioning may reduce the effectiveness of postural support.
- These products are not intended for use as vehicle occupant restraints.
- Regular skin inspection is recommended for users with reduced sensation, fragile skin or limited mobility.
- Shear and moisture can contribute to skin damage.
- Ensure belts and harnesses are fitted securely but do not restrict breathing, circulation or safe movement.
- Keep away from sharp objects, excessive heat and open flames.

Cleaning & Maintenance

- Remove any surface contamination before cleaning.
- Clean using approved household or hospital-grade sanitising cleaners in accordance with local infection control guidelines.
- Ensure all cleaning residue is removed where appropriate.
- Allow products to fully dry before reuse or storage.
- Do not store products when wet or damp.

Inspection

Before use, check:

- Secure attachment of all straps, buckles and fixings
- Correct positioning and adjustment
- Signs of wear, fraying or degradation
- Cleanliness and integrity of the product.

Storage & Transport

- Store in a clean, dry environment away from direct sunlight and excessive heat.
- Avoid prolonged exposure to extreme temperatures during storage or transport.

Incident Reporting

Any serious incident relating to the use of this product should be reported to Gel Ovations Europe Ltd.

Disposal

Dispose of products and packaging in accordance with local and national regulations. Products contaminated with bodily fluids should be disposed of in accordance with local clinical waste procedures.

Product Information

Products are supplied NON-STERILE unless otherwise stated.

Service Life

Service life will depend on frequency of use, fitting conditions, cleaning regime and environment.

Intended Use

Gel Ovations Made to Measure products are designed to provide customised pressure redistribution, positioning, comfort and protection solutions tailored to an individual user's needs, seating system or clinical requirements. Products should be prescribed, specified or approved by a qualified healthcare professional where appropriate.

Product Information

Made to Measure products are individually manufactured to customer specifications and may vary in size, shape, thickness, mounting method, cover type, hardware configuration and pressure redistribution properties. Custom products may include dimensional gel, flat gel, foam combinations, vapour-permeable covers, straps, hardware or specialist mounting systems.

Instructions for Use

- Ensure the product supplied matches the agreed specification before use.
- Check that the product is securely positioned and stable before use.
- Ensure that straps, fixings, hook and loop fastening or mounting hardware are correctly attached where applicable.
- Position the product as instructed by the prescribing clinician or healthcare professional.
- Regularly assess comfort, posture and skin condition during use.
- Any modifications to the product after manufacture should only be undertaken by Gel Ovations Europe Ltd or an appropriately qualified professional.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, damage, loose fixings or degradation.
- Discontinue use if the product becomes damaged or compromised.
- Clinical supervision is recommended for users with high-risk pressure care needs.
- Incorrect positioning or use may reduce the effectiveness of pressure redistribution.
- Shear and moisture can contribute to skin damage.
- Custom products are manufactured for the intended individual or application and may not be suitable for other users.
- Made to Measure Custom-made products may include product-specific fitting or cleaning instructions supplied separately.

Surgical Pressure Care Products

Intended Use

Gel Ovations Surgical Pressure Care products are designed to assist with pressure redistribution, positioning, comfort and protection during surgical, procedural and clinical applications. Products are intended to help reduce pressure, shear and friction on vulnerable anatomical areas during periods of prolonged positioning. Products should be selected and used by appropriately trained healthcare professionals following individual clinical assessment and local clinical protocols.

Includes but is not limited to surgical head rings, armboards, heel protectors, positioning wedges and operating table pressure care products.

Instructions for Use

- Ensure the product selected is appropriate for the intended procedure, positioning requirement and patient needs.
- Position the product securely on the operating table, trolley or clinical surface before patient transfer.
- Ensure that the gel surface is correctly aligned with the vulnerable anatomical area requiring pressure redistribution or protection.
- Confirm that all positioning devices remain stable throughout use.
- Avoid folds, wrinkles or uneven positioning beneath the patient.
- Reassess patient positioning regularly during prolonged procedures in accordance with local clinical guidance.
- Products should only be used by trained healthcare professionals.

Warnings & Precautions

- Products should be regularly inspected for signs of wear, puncture, tearing, fluid ingress or degradation.
- Discontinue use immediately if the product becomes damaged or compromised.
- Incorrect positioning may reduce the effectiveness of pressure redistribution and patient protection.
- Prolonged pressure, shear and moisture may contribute to skin damage and pressure injury.
- Care should be taken when positioning patients with fragile skin, reduced circulation or high-risk pressure care needs.
- Ensure that products do not interfere with surgical access, airway management or patient safety systems.
- Do not expose products to sharp surgical instruments or excessive heat sources.

Warranty

Products are warranted against defects in materials and workmanship for one year.

Warranty does not cover:

- Misuse
- Alteration
- Incorrect cleaning
- Normal wear

Warning: Shear and moisture are unhealthy for skin. These products are designed with a moisture-impermeable cover. If used in wet conditions, please dry the product off before continued use. If used in wet conditions, please dry for an additional 10 minutes after surface drying before continued use. This particularly applies to arm and footrests, where pressure can be more concentrated.

Gel Ovations Europe Ltd
Charlton Road
Bristol BS10 6NF
United Kingdom

Tel: +44 (0)1454 285 071
Email: info@gelovationseurope.com
Visit: www.gelovationseurope.com

#StopThe Pressure

Copyright 2026 All contents copyright Gel Ovations Europe Ltd. All copyright, design rights and other intellectual property in Gel Ovations products and designs are and remain the property of Gel Ovations Europe Ltd. All product details correct at time of going to print. Due to continual product development we reserve the right to change specifications or materials without prior notice.

VAT Number: 921 3722 49
Company Number: 6362508

Issue June 2026